
Sub-2 μm Silica Particles in Chiral Separation

Diana Ibrahim and Ashraf Ghanem

Additional information is available at the end of the chapter

<http://dx.doi.org/10.5772/intechopen.79063>

Abstract

For decades, the race for the shortest chromatogram with the best resolution and separation efficiency has been the focus of researchers and manufacturers. Considerable advancement has been attained in the field of separation science with the widespread applications and outstanding performance of nanomaterials. According to the van Deemter equation, sub-2 micron particles employed in a conventional HPLC short column should subsequently result in analysis time reduction and efficiency improvements without the drawbacks of high pressure associated with sub-2 micron particles. This chapter provides comprehensive discussion about the applications of the new sub 2 microns silica particles in chiral separation of racemates.

Keywords: CHIRALPAK IG-U, HPLC, chiral separation, sub-2 micron, nanomaterials

1. Introduction

1.1. Nanomaterials as stationary phases in separation science

Nanomaterials are nanostructures with sizes in the range of approximately 1–100 nm [1]. These nanomaterials frequently have chemical and physical characteristics that are distinct from those of their macroscopic counterparts [1]. They can be exploited in many fields of science and technology including separation science [2]. In separation science, this term often refers to nano-materials-based stationary phases used to separate chemical compounds [2]. Widespread applications and outstanding performance of nanomaterials have not only accelerated the development of separation science, but also offer many opportunities in other related disciplines, and have a significant impact on many fields of science [2, 3]. Separation science is based on the application of broad chromatographic techniques to achieve separations of compounds. Such separation is achieved by regulating the magnitude of the distribution

coefficient between two distinct phases namely the stationary and the mobile phases [1–3]. The components separate as they migrate with different rates depending on their unique distribution coefficients, they separate [4]. Different chromatographic techniques are available depending on the type of the phases [4]. The chromatography is known to be liquid chromatography (LC) when it employs a liquid mobile phase [5]. The most sophisticated form of LC is High-performance liquid chromatography (HPLC) where the mobile phase passes through the stationary via a pump at high pressures [4, 5].

2. Applications of nanomaterials in HPLC stationary phases

In conventional HPLC, the stationary phase (SP) plays a pivotal role in the separation technique [5]. The packing particles constituting the SP are of several micrometres in diameter with nanometre-sized pores [6]. Therefore, the industry has pushed researchers to investigate new packing materials as an attempt to achieve high throughput with robust analysis [6]. Packings in HPLC can be divided into three types-polymeric, inorganic, and hybrid materials. At present, inorganic materials, which include silica, hydroxyapatite, graphite, and metal oxides, etc. are widely used in research and applications [7]. Among these materials, silica is almost ideal support given its favourable characteristics, for example, good mechanical strength, high chemical and thermal stability, controllable pore structure and surface area, etc. [7]. Therefore, silica has been developed as the most widely used HPLC packing material [6, 7]. Throughout the years, many silica stationary phases (both porous and non-porous) have been commercialised and widely applied for analysis of pharmaceutical and biological samples [8].

2.1. Porous and non-porous nanomaterials

Non-porous and porous particles are the two major types of spherical packing materials used in HPLC [8]. The significant difference between both particles is that porous particles

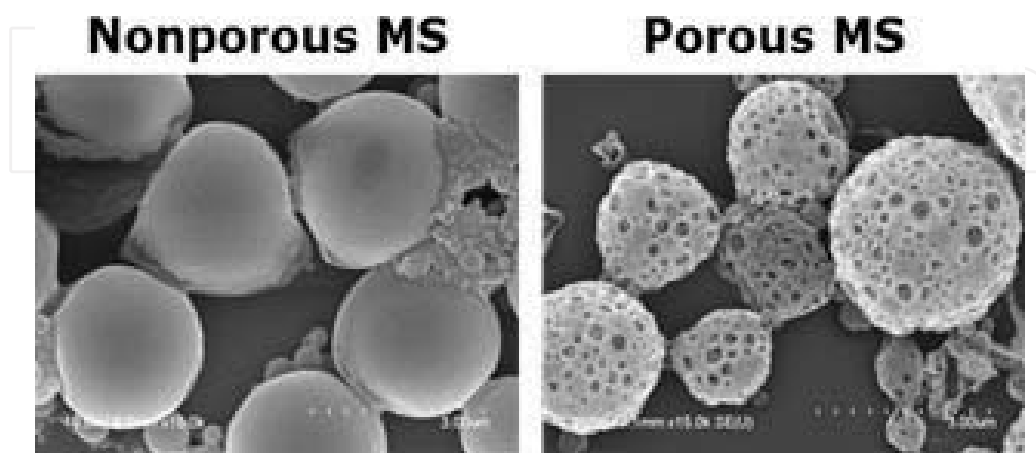


Figure 1. The difference in surface area between porous and non-porous microspheres under scanning electron microscopy [2].

have resistance to mass transfer contribution from the stagnant mobile phase in the pores [8]. Decreasing the particle size and increasing the diffusion coefficient can improve the mass transfer of solutes in the mobile phase [3, 5]. Non-porous particles can provide lower mass transfer resistance and higher efficiency than porous particles [8]. However, porous particles have higher surface areas (**Figure 1**) and can provide much higher sample loading capacity [8].

On the other hand, in porous particles, solutes transfer from the mobile phase exterior to the particles into the mobile phase within the pores to interact with the chiral stationary phase (CSP) [9]. Following this interaction, the solute molecule must diffuse out of the particle and continue its journey down the column ahead of the solute [5, 9]. This slow rate of mass transfer into and out of the porous particle is a source of HPLC band broadening [9]. **Figure 2** illustrates a reduction in particle size shortens the path length of this diffusion process, improves mass transfer, and provides better efficiency [9].

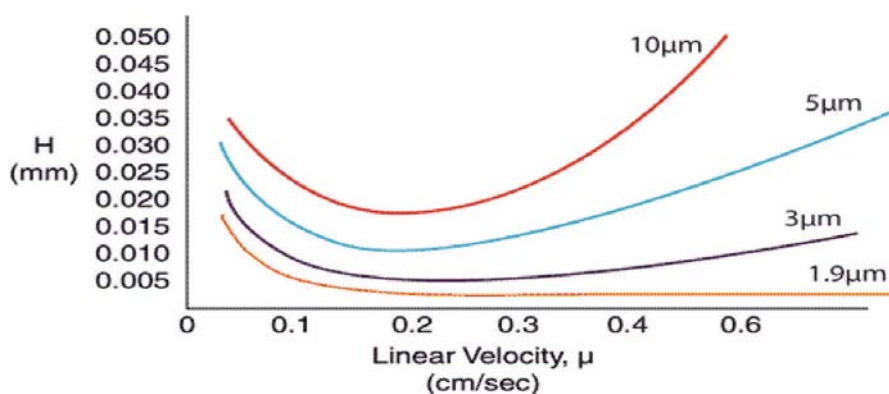


Figure 2. Smaller particle sizes increase efficiency and result in a wider range of flow rates [9].

3. Effect of particle size on the separation efficiency, speed and resolution of chiral separations

3.1. Relationship between particle size, and column efficiency

Particle size is known to be the mean diameter of the spherical support employed in column packing [6]. This physical dimension significantly impacts HPLC column performance [9]. A decrease in particle size increases peak efficiencies (**Figure 2**). This is based on the resolution equation (Eq. (1)) which comprise of three terms: selectivity, retention capacity, and efficiency [10]. The components of an analytical method alter each of these terms. In particular, the column's particle size affects the efficiency factor from the equation [10]. Efficiency is a qualitative term used to measure the number of theoretical plates in a column. Put simply, as particle size is lowered, efficiency increases, and more resolution is achieved [10].

$$R_s = 2(t_{R,2} - t_{R,1}) / (w_{b,1} + w_{b,2}) \quad (1)$$

Burns et al. observed a nearly linear correlation between the width of the particle size distribution of commercially available HPLC particles and the minimum reduced plate height, the van Deemter equation (VDE) A-term and the minimum reduced separation impedance [10, 11]. Column efficiency in HPLC is influenced by a number of factors such as particle size, flow rate and degree of cross-linkage of gels [12]. Particle size distribution (PSD) of packing materials is also considered one of the important factors [12]. It has been empirically found that column efficiency is improved by narrowing the PSD [11, 12]. Because the greatest the achievable plate height is, the more effective the PSD has on the separation efficiency [12]. On one side, column efficiency or plate number is dependent on particle size, and the pore size controls the surface area where retention is controlled primarily by the surface area [9–12].

3.2. The impact of the pore size of silica gel on the CSPs

Retention is directly related to surface area; therefore, the use of large-pore columns is not desirable when small-pore columns can be used [13]. Selection of the pore size is based on providing easy access for the molecules to the pores in the column [10–12]. Consequently, the higher surface area associated with small pore-columns is preferred mainly because the analytes are small enough to pass through the pores [12, 13].

The performance of the CSP increases with pore size when the pore diameter is large enough for the penetration of macromolecules [13]. Specific surface area and, therefore, the number of silanol groups on the surface of the silica gel, decreases with increasing of pore size; consequently, the bound amount of the chiral selector depends on the pore size of silica matrix [13]. The particle size of silica gel has a major effect on the performance of the column, increasing the particle size from 3 to 10 μ decreased the theoretical plate number [13]. A reduction in particle size can lead to more compact and stable packing and thus better column efficiency.

3.3. Chromatographic effects of varying particle size and size distributions

In the late 1960s, Horvath and coworkers introduced columns packed with rigid pellicular particles (40–50 μ) applicable under high pressures [14]. The thin porous coat allowed for robust solute mass transfer through the packing, hence, improving column efficiency. However, pellicular particles had a drawback of low sample capacity [16]. In the 1970s, large porous/pellicular particles were reduced down to smaller porous particles of 10 μ to eliminate the drawbacks of pellicular materials [16]. However, particles of silica smaller than 40 μ have demonstrated some difficulties with packing reproducibility [17]. Irregular shapes of microporous particles were used throughout the 1970s until the spherical material was obtained and improved. In the 1980s, 5 μ became the standard particle diameter, and in the early 1990s, 3–3.5 μ particle diameters were also commercially available [16, 17]. The latter demonstrated 30–50% faster analysis times and higher efficiencies compared to 5 μ . Methods can be easily transferred from 5 μ to similar 3 stationary phases [14–17] (Figure 3) [15].

History of HPLC Particle Development







Year(s) of Acceptance	Particle Size	Most Popular Nominal Size	Plates / 15cm
1950's		100 μm	200
1967		57 μm (pellicular)	1,000
1972		10 μm	6,000
1985		5 μm	12,000
1992		3.5 μm	22,000
2003		$\leq 2\mu\text{m}^*$	>30,000

Figure 3. The reduction of particle packing throughout the years in hope for the shortest fastest chromatogram [16].

4. Small-particle (sub-2- μm) columns for high efficiency and speed

Separation efficiency is inversely proportional to the stationary phase diameter [17]. Stationary phase manufacturers have reduced particles for packing down to micron-sized [17]. If packing materials could be further reduced in the future down to the nanometre scale, the band dispersion would consequently be reduced further by 6 magnitude orders [17, 18]. As a consequence, in 2004, the first available porous silica with small particle size was commercialised (1.7 μ), which allowed better resolution compared to the current 5 or 3.5 μ [18]. Several column suppliers now offer columns packed with particles in the range of 1.5–2 μ [18]. The term sub-2 micron, including particles of 2 μ , is used in this work for the sake of clarity [19]. Different works, dealing with drug and metabolites analysis, bioanalytical as well as environmental separations, compared columns packed with 5 μ and sub-2 micron supports and demonstrated that the latter clearly reduced the analysis time with comparable efficiency [20]. However, the quest towards the use of nanomaterials in chromatography has encountered serious challenges such as extremely high back pressures and problems associated with frits [20, 21].

The high back pressure is induced by the friction of the mobile phase percolating through the sub-2 μm particles stationary phase, generating heat that can be detrimental to the separations [22]. Studies suggest that reducing column internal diameter (i.d.) minimised frictional heating effect from the radial temperature gradient [22, 23]. This is due to fast heat dissipation within such a narrow-bore column [23]. As column length is proportional to the particle size, shortening the columns lead to fast separation with sub-2 μm particles [23].

As shown in **Figure 4**, sub-2 micron particles are noted to be highly efficient and hence, the column length can be shortened while maintaining resolution in a shorter analysis time [23]. To achieve fast separations, short columns and high flow rates are necessary. In such columns, it can be practically difficult to achieve axially and radially homogenous beds [24]. It seems more logical to use smaller diameter columns, such as 3 mm i.d. when using sub-2 micron particles [23, 24]. This significantly reduces the flow rate required to achieve optimum efficiency, which in turn minimises the extra-column dispersion caused by the tubing [25]. Higher linear velocities can be achieved at lower flow rates, with much lower pressure drops in the tubing [25].

If the main goal is reducing analysis time, an increase in the flow rate above the optimum rate allows for robust separations, while maintaining resolution due to the small particles lower mass transfer resistance [24]. On the other side, if the primary goal is higher resolution, maintaining column length can increase resolution with a subsequent increase in analysis time [24]. Particle size reduction has more effect than column length, gradient time, or flow-rate to improve peak capacity in gradient mode [26]. However, these small particles can generate a high bp incompatible with conventional instrumentation [27]. It is evident that a reduction in particle size reduces backpressure because of the inverse square relationship between them [27]. As a result, new HPLC instrumentation such as ultra-high performance liquid chromatography (UHPLC) has been developed to handle elevated pressures above 400 bar [27]. However, employing shorter columns with smaller particles (i.e. sub-2 micron) have the ability to combine high resolution without exceeding the pressure limit of 400 bar associated with conventional HPLC [23–27].

4.1. Van Deemter analysis of sub-2 micron CSPs

According to VDE, the A- and C-terms are directly proportional to the particle size [28]. Therefore, the use of smaller particles provides a decrease of the plate height together with a flatter profile of the right branch of the van Deemter curve [28]. A reduction in column i.d. results in less chromatographic dilution and, consequently, increased concentration of the injected sample on LC system [25]. The chromatographic dilution increases proportionally

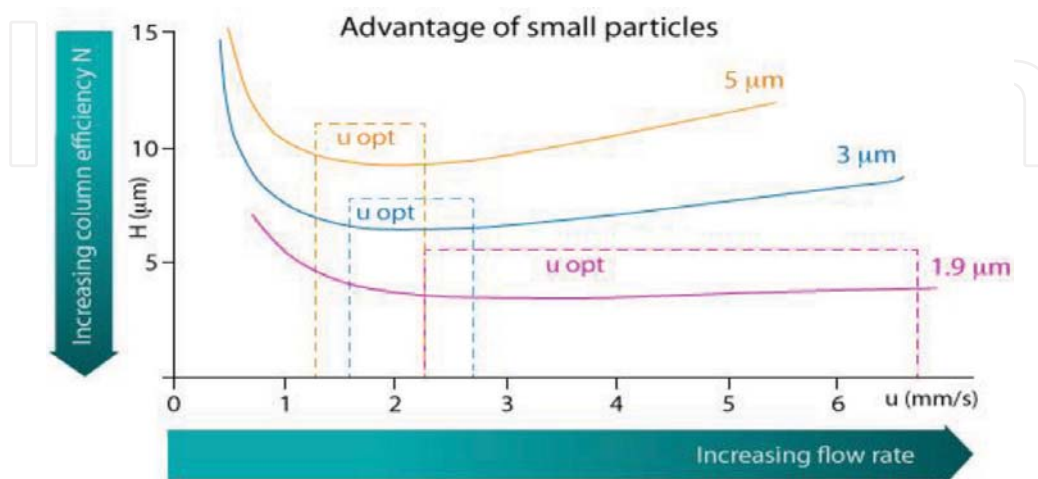


Figure 4. A reduction in particle size results in an increase in column efficiency, a wider range of flow rates is applicable for small particles [23].

with the square of the column radius and with the square root of column length [29]. Thus, a reduction in column diameter results in a significantly lower dilution factor, thereby increasing the concentration in the eluted peak [29]. Downscaling the column used in an analytical method should result in an almost 4000-fold gain in sensitivity [28]. With the reduction in particle size, column efficiency improved further allowing a reduction in column length. Shorter columns are now in vogue [28]. Not only does a shorter column provide faster separations but also solvent use is reduced [28]. Columns of 50 mm in length now provide plate counts formerly obtained on 15- and 25-cm columns packed with larger particles [25, 28, 29]. The sub-2- μm columns have struck the fancy of those who wish to decrease their analysis times by shortening the column length and to those who want to have greater plate count by using longer columns, albeit at the higher pressure [25, 28, 29].

The equation demonstrated the obvious advantage of using small particles to decrease plate height [30]. The chromatographic separating power of HPLC is dependent upon the selectivity of the mobile/stationary phase and the efficiency of the column [12, 13]. The column efficiency is dependent upon multiple factors most importantly: the column length and the packing particle size together with the mobile phase velocity [22]. At a fixed velocity, the column efficiency increases in direct proportion to the column length [24]. At the minimum of the plate height versus velocity curve, the column efficiency increases in inverse proportion with the particle size [22, 24].

As seen in **Figure 5**, van Deemter equation describes that efficiency varies with the linear velocity, and the nature of the second and third terms of the equation indicates a minimum value for plate height (HETP) [31]. In the third term of van Deemter equation, the particle size is squared, and so the curve is steeper for larger particles at high linear velocities [31]. The A term depends

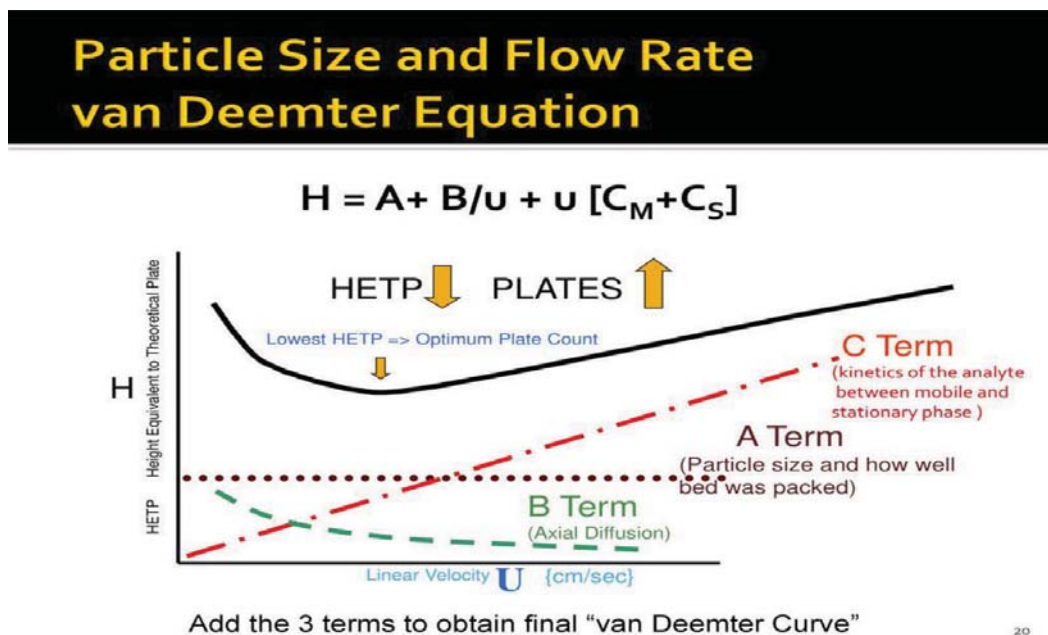


Figure 5. Van Deemter equation describes that efficiency varies with the linear velocity, and the second and third terms indicates a minimum value for HETP [31].

on both the quality of the column packing and the contribution values of the coefficients A, B and C for the different columns, can be accounted for by the minor contribution of several effects (packing characteristics and the combined effects of frictional heating and high pressure) on the velocity-dependence of the plate height. B- and C-terms of the equation depend on analyte retention [32]. The B-term is expected to increase with analyte retention as more time is available for diffusion to take place in the mobile phase [32]. According to the theory, smaller particles should perform lower plate heights and higher optimum linear velocity [31, 32].

The dependence of the third term (C-term), is considered to represent mainly the resistance to mass transfer in the mobile phase, on the square of the particle size translates into a substantial decrease in the plate height with smaller particles, especially at high linear velocities [33]. Small particle diameters induce an increase in efficiency, optimal velocity and mass transfer. Sub-2 micron particles packed into shorter column permit shorter analysis time along with using less solvent without compromising the resolution between closely eluting peaks [34]. Because the H-u curves are flatter (lower C term) for the smaller particle diameters, they also allow conducting separations at linear velocities higher than the optimum without significant loss of efficiency [34]. Using small diameter packing material reduces eddy diffusion and mass transfer resistance in the mobile phase [28, 33]. Van Deemter realised a correlation between increasing peak efficiency and a reduction in particle size [28, 34].

Optimization of efficiency and analysis time can be useful but generally leads to a large increase in the analysis time [35]. Instead, tuning the column length together with the stationary phase morphology (e.g. particle size) can result in a better compromise between the plate count and analysis time [36, 37]. Column length and plate count are related through the height equivalent to one theoretical plate with the relationship between the theoretical plate and mobile phase velocity described by VDE as the sum of different band-broadening contributions [34–36].

Based on VDE, the solution for enhancing chromatographic performance is to use shorter columns with small particle diameters (i.e. sub-2 micron particles) to induce a simultaneous improvement in efficiency, optimal velocity and mass transfer. The use of these sub-2 micron materials in LC is examined, including their applications in normal-phase LC, reversed-phase LC. In this study, the possibilities and restrictions of chromatographic separations obtained with 5 cm long bore columns packed with sub-2 micron particles is presented. Performance of columns immobilised on silica gel with different internal diameters and different lengths will be briefly mentioned to provide an overview of the miniaturisation of HPLC column technology.

5. Performance of CHIRALPAK IG-U®: In terms of enantioselectivity and solvent versatility

In recent years, column miniaturisation has been investigated and tested in order to achieve highly sensitive chromatography [38]. The miniaturised columns are better for handling minute and/or dilute samples, especially in an area such as forensic science and sport drug trails [38]. The idea of miniaturisation is to provide higher sensitivity and peak capacity than standard columns with minimal dead volume for small sample amounts [39]. Narrow-bore

columns are used on a conventional HPLC system [24]. The sub-2 micron silica-based stationary phases have established themselves as an effective analytical tool in achiral applications, but in the field of chiral separations, the technology related to the development of sub-2 micron CSPs is still not used in the market on conventional HPLC [40–43].

Daicel group recently commercialised a sub-2 micron 5 cm column applicable for use on conventional HPLC [44]. The design is based on the simple way of reducing solvent usage by using a shorter column. A more dynamic saving in solvent usage is made by reducing the i.d. of the column, together with an appropriate scaling down in the flow rate [44]. Separation efficiencies are also recovered by reducing particle size down to sub-2 micron; because columns packed with sub-2 micron particles offer advantages over the more traditional systems containing 3 and 5 micron particles by allowing operation at higher flow rates without compromising efficiency [45]. Consequently, this results in shorter analysis times and a reduction in solvent consumption, together with associated improvements in resolving power, sensitivity and peak capacity [45].

Ghanem et al. [46] investigated the impact of reducing the three VDE parameters (Length, i.d. and particle size) on separation and efficiency via the transition from conventional CHIRALPAK IG[®] to the sub-2 micron CHIRALPAK IG-U[®]. The effects of miniaturising the three column parameters (i.d., length and particle size) five times from CHIRALPAK IG[®] (250 mm length, 4.6 mm i.d., and 5 mm particle size) to CHIRALPAK IG-U[®] (50 mm length, 3 mm i.d., and 1.6 μm or sub-2 micron particle size) using similar CSP amylose *tris* (3-chloro-5-methylphenylcarbamate) for the enantioselective separation of racemates under normal standard, non-standard organic phase, and reversed-phase chromatographic conditions are discussed below [47].

Pore size influences several factors such as: the retention factor, the separation factor, and the resolution of racemates was also examined. CHIRALPAK IG-U[®] has been tested in normal-phase mode chromatographic separation consisting of *n*-hexane/ethanol screened from 90:10 to 10:90 v/v at 1 mL/min flow rate on CHIRALPAK IG-U[®] at fixed UV detection 245 nm. Out of the twenty-eight compounds tested, eleven compounds (Naftopidil, Naproxen, Indoprofen, Cizolitrine, Carprofen, Miconazole, Nomifensine, Tocainide, Propafenone, Flavanone, and 6-Hydroxyflavanone) were partially, or baseline separated under either 90:10 or 80:20 v/v *n*-hexane/ethanol mobile phase. Substituting ethanol (EtOH) with 2-propanol (2-PrOH) resulted in the separation of only seven compounds (Naftopidil, Carprofen, Sulconazole, Propafenone, Flavanone, 6-Hydroxyflavanone, and 1-Acenaphthenol) under either 90:10, 80:20, 70:30 or 60:40 v/v *n*-hexane/2-PrOH. Regarding resolution (R_s) and separation factor (α), EtOH in mobile phase system showed better results than 2-PrOH where (Naproxen, Indoprofen, Miconazole, Nomifensine, and Tocainide) were all separated when 2-PrOH was replaced by *n*-hexane (See **Figure 6** for examples). This is mainly because the mobile phase travels easily in large spaces between particles and hence particle size affect permeability; smaller particles can be packed closer together, thus, using ethanol resulted in the best separation with the highest resolution and separation factor [46, 47].

CHIRALPAK IG-U[®] showed great performance in different solvents such as non-standard solvents namely dichloromethane, tetrahydrofuran and Methyl *tert* Butyl Ether [46]. The

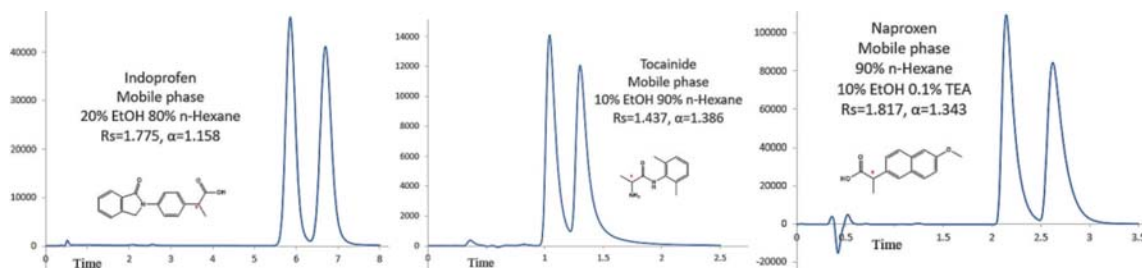


Figure 6. The effect of EtOH in mobile phase composition on Indoprofen, Naproxen, and Tocainide.

addition of non-standard solvents in mobile phase composition enhanced resolution and separation in several tested racemates for example, in case of Tocainide, R_s 1.44 and α 1.39 in standard solvents namely *n*-hexane/EtOH 90:10 *v/v* were enhanced to R_s 1.89 and α 1.66 when using non-standard solvent in mobile phase composition (*n*-hexane/DCM/EtOH 50/50/0.2 *v/v/v*) (**Figure 7**) [47]. Of interest, compound 1-phenyl-2,2,2-trifluoroethanol which was not resolved under any standard solvents' combination investigated, was baseline separated under non-standard organic solvent (MtBE/EtOH 40/60% *v/v*) with R_s 1.55 and α 1.78. Similarly, compounds Aminoglutethimide and α -Methyl DOPA were only separated under non-standard organic mobile phase composition (MtBE/EtOH 40:60 *v/v*) and (*n*-hexane/DCM 85%/15% *v/v*) [47]. The chiral recognition of sub 2-micron column CHIRALPAK IG-U[®] is like that of CHIRALPAK IG[®] where polarity is playing a role. Another reason might be the stereo environment of the chiral cavities in amylose derivatives which might be favorable in the presence of ethanol. Other researchers have speculated that the configuration of the chiral cavities in the amylose tris (3,5-dimethylphenyl carbamate) is determined by the composition of mobile phase in normal phase mode while the configuration of reversed phase mode remains unchanged. It is of essential to note that the chiral recognition is due to different factors such as hydrogen bonding, π - π interactions and the chiral cavities of CSPs with specific configuration responsible for bonding of varying magnitude between the stationary phase and enantiomers [46, 47]. CHIRALPAK IG-U[®] was investigated under reversed-phase conditions including ACN and H₂O ranging from 10 to 90% (*v/v*) [46]. The resolution and separation factors were enhanced in several compounds compared to other separations

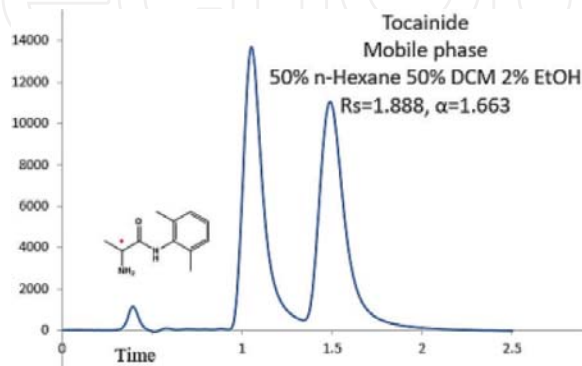


Figure 7. Tocainide resolution and separation factor were enhanced from (R_s :1.44 and α :1.39) under standard solvent (*n*-hexane/EtOH 90:10 *v/v*) to (R_s :1.89 and α :1.66) under non-standard solvent (*n*-hexane/DCM/EtOH 50:50:0.2 *v/v/v*).

achieved under standard and non-standard organic solvents. For example, few separations were achieved for compounds (Naftopidil, Miconazole, Sulconazole, Aminoglutethimide, Tocainide, Propafenone, Flavanone, and 6-Hydroxyflavanone). Compound Naftopidil was baseline separated with a R_s of 2.56 and α 1.62 under (ACN/H₂O/TEA 80:20:0.1% v/v/v) (**Figure 8**) [47]. Similarly, in case of compound Aminoglutethimide; R_s 1.90 and α 1.34 were superior to other separations achieved under standard and non-standard organic solvents. Compound 6-Hydroxyflavanone which was separated under standard and non-standard solvents, was separated under reversed phase condition (ACN/H₂O/TEA 40:60:0.1% v/v/v) with superior R_s 2.39 and α 2.71 (**Figure 8**) [47].

According to the following results and VDE Ghanem et al. [46, 47] and VDE, all three parameters (length, i.d., and particle size) reduced in the transition from conventional CHIRALPAK IG[®] to the sub-2 micron CHIRALPAK IG-U[®] resulted in an enhanced separation and resolution (**Figure 9**). However, Practical difficulties that one can expect following the sub-2-micron particle approach are twofold: one is inherently related to the decrease of column permeability

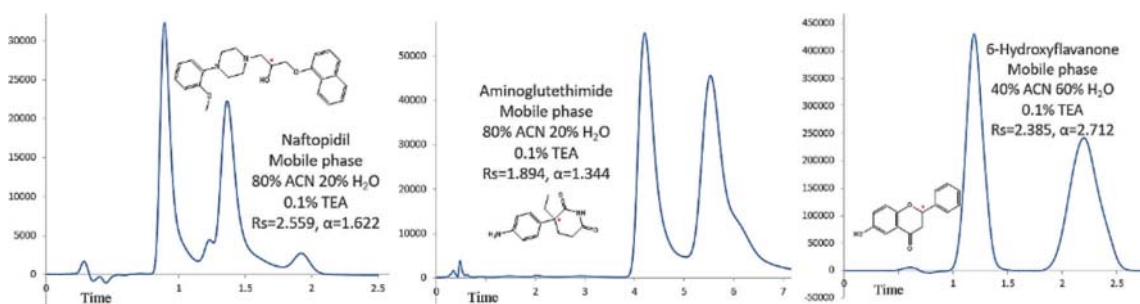


Figure 8. Naftopidil was baseline separated with a R_s of 2.56 and α 1.62 under reversed phase solvent composition (ACN/H₂O/TEA 80:20:0.1% v/v/v). Aminoglutethimide with R_s 1.90 and α 1.34 were superior to other separations achieved under standard and non-standard organic solvents. Compound 6-Hydroxyflavanone which was separated under standard and non-standard solvents, was separated under reversed phase condition (ACN/H₂O/TEA 40:60:0.1% v/v/v) with superior R_s 2.39 and α 2.71.

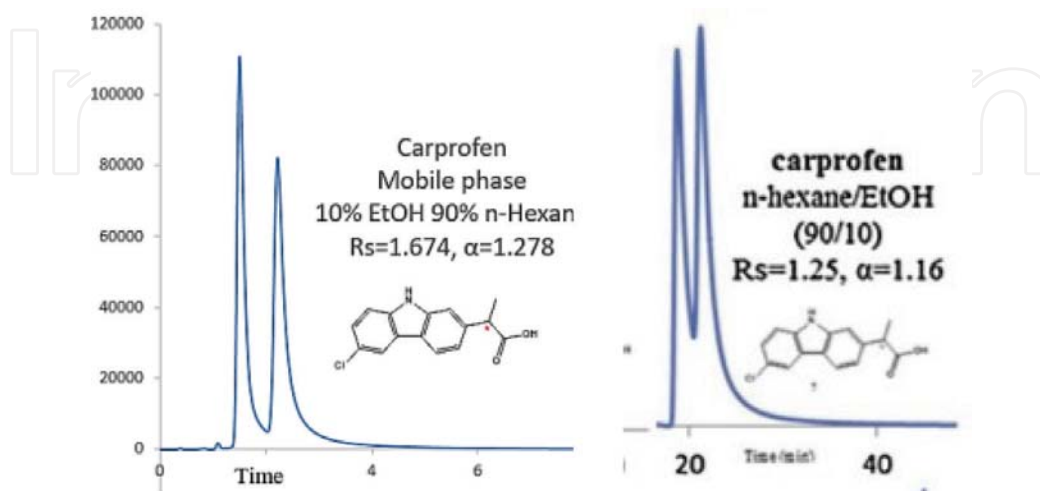


Figure 9. CHIRALPAK IG-U[®] (left side) shows enhanced separation and resolution in shorter time of 2 minutes compared to 20 minutes using the CHIRALPAK IG[®] (right side).

that accompanies the particle size reduction; the other one is associated to the adaptation of the surface modification chemistry of classical CSPs to smaller particles [21–26].

The column permeability reduction is linked to the increase in pressure that is proportional to the inverse of the particle diameter squared: thus, reducing the particle diameter by a factor of 3 will result in a ninefold increase in the column back pressure [48]. As a consequence, depending on the column length and eluents viscosity, the full potential of high-speed separations can only be exploited on chromatographic hardware that can withstand elevated pressures (UHPLC) [49]. An additional complication may arise from the pronounced propensity of the smaller particles to aggregate during synthetic steps leading to a final stationary phase with non-optimal performances primarily regarding permeability and/or efficiency [18]. Mechanical resistance and long-term stability of the packed bed are also of significant concern when high flow (and hence high pressure) applications are planned [18].

This area needs considerable attention as solvent efficient narrow-bore columns have already become mainstream for ‘greener’ chromatography [50]. For ultrafast separations, the sub-2- μm totally porous particles provide better solutions [18, 48]. Thus it can be a viable option to achieve ultrafast separations with slightly lower efficiency, but without a large investment in ultrahigh-pressure instruments [49].

6. Future perspectives

Instruments have been trying to follow the footpath of column developments [51]. The life cycle for instrument development is much longer than what is required for new packings and columns [52]. An area that has been delaying further improvements in column efficiency is the instrument contribution to band dispersion associated with HPLC and UHPLC instruments and their column-instrument interface designs [53]. Integration of column hardware and instrument connections are essential to eliminate dead volumes, much like what has been achieved in some nano and chip instruments [53]. The area of frit and end fitting design needs attention since the column packing where the separation takes place should be located at or near the injector device and the detector measurement device [52, 53]. This may necessitate a new column design that not only cuts down on this extra-column volume but can handle higher pressures associated with smaller particles [53].

Reducing the column i.d. is the first of several critical steps in miniaturising a LC system. Extra column peak broadening must be reduced accordingly to preserve optimal performance [54]. Excessive extra column band-broadening causes considerable loss of separation efficiency and, thereby, sensitivity. Connection tubing should be kept as short and especially as narrow as possible to minimise extra column band broadening and result in an acceptable increase in back pressure [35, 54]. Making connections with silica capillaries can be a challenge to less-experienced users and often has been considered the most difficult part of setting up a nano-liquid chromatography (nano-LC) system [55]. LC system implies that all system components should be downscaled, including column, connecting tubing, connections, injector, and the interface to the detector [55]. Nano-LC columns typically require flow rates of 500 nL/min or less [35]. Achieving reproducible flow and gradient formation requires dedicated approaches.

Ideally, the flow should not be split and used directly from the pump as it is used in standard HPLC [35]. These nano-LC systems are often called splitless systems and are commercially available [53]. The direct flow systems can be divided into two groups: the 'solvent refill' systems and the 'continuous flow' systems [53]. Commonly, these systems also are capable of operating at UHPLC pressures. Whereas UHPLC is mostly used to increase throughput in standard-bore LC, its use in nano LC is mainly aimed at improving separation efficiency through the use of longer nano-LC columns packed with 2- μm (or smaller) particles [53].

Further miniaturisation of standard UHPLC instrumentation is possible [50]. Microfluidics has proven a great success as an alternate approach to achieve analytical separations [48]. Such downsizing of the LC experiment would undoubtedly require a major redesign in the column and instrumentation [51, 54]. The use of miniaturised instruments would result in a significant solvent, bench-space, and sample savings, and with mass spectrometry would allow even better interfacing [35, 53–55]. Chip-based LC systems have been extensively investigated, and a limited number of instruments have already been commercialised [55]. However, the adoption rate for commercial instruments has been somewhat slow and, compared to regular analytical columns, in microfluidics column efficiencies are not as high as expected [54]. The packing of microparticles within narrow channels is difficult, and one of the reasons for low column efficiency in microfluidics-based column systems [18, 35, 50–55].

7. Conclusion

Chromatographic technique development has always strived towards higher efficiency and more rapid resolution in diverse areas such as clinical, pharmaceutical and toxicology analysis, as well as enantioselective separation, to reduce costs and enhance throughput. Conventional HPLC, could not fully satisfy these requirements due to the relatively low efficiency and lengthy analysis time. Several approaches have been undertaken to achieve these goals, such as increasing flow rates and shortening the column length by using monolithic columns. However, these approaches may result in low phase ratio and low capacity factor. One promising approach is to use smaller size silica particle (less than 2 μm , as compared to conventional 3 and 5 μm size column packing materials. This is motivated by VDE that shows an inversely proportional relationship between the separation efficiency and particle size. Therefore, nano-or sub-micron size supporting materials may be promising to improve separation efficiency.

Abbreviations

CSP	chiral stationary phase
HETP	plate height
HPLC	high-performance liquid chromatography
i.d.	internal diameter

LC	liquid chromatography
Nano-LC	nano-liquid chromatography
PSD	particle size distribution
SP	stationary phase
UHPLC	ultra-high performance liquid chromatography
VDE	Van Deemter equation

Author details

Diana Ibrahim and Ashraf Ghanem*

*Address all correspondence to: ashraf.ghanem@canberra.edu.au

Chirality Program, School of Science, Faculty of Science and Technology, University of Canberra, Australia

References

- [1] Beeram S, Rodrlguez E, Doddavenkatanna S, Li Z, Pekarek A, Peev D, Goerl K, Trovato G, Hofmann T, Hage D. Nanomaterials as stationary phases and supports in liquid chromatography. *Electrophoresis*. 2017;**38**:2498-2512. DOI: 10.1002/elps.201700168
- [2] Nesterenko E, Nesterenko P, Connolly D, He X, Floris P, Duffy E, Paull B. Nano-particle modified stationary phases for high-performance liquid chromatography. *The Analyst*. 2013;**138**:4229. DOI: 10.1039/c3an00508a
- [3] Sierra I, Perez-Quintanilla D, Morante S, Ganan J. Novel supports in chiral stationary phase development for liquid chromatography. Preparation, characterization and application of ordered mesoporous silica particles. *Journal of Chromatography. A*. 2014;**1363**:27-40. DOI: 10.1016/j.chroma.2014.06.063
- [4] Sekhon S. Bhupinder, Enantioseparation of chiral drugs-an overview. *Journal of ChemTech Research*. 2010;**2**:1584-1594
- [5] Fekete S, Veuthey J, Guillarme D. Comparison of the most recent chromatographic approaches applied for fast and high resolution separations: Theory and practice. *Journal of Chromatography*. 2015;**1408**:1-14. DOI: 10.1016/j.chroma.2015.07.014
- [6] Zhi-Jian H et al. Chiral stationary phases and their relationship with enantiomer structures in Enantioseparation research of analytical laboratory. *Journal of the Mexican Chemical Society*. 2014;**59**:43-49. DOI: 10.29356/jmcs.v59i1.13

- [7] Qiu H, Liang X, Sun M, Jiang S. Development of silica-based stationary phases for high-performance liquid chromatography. *Analytical and Bioanalytical Chemistry*. 2011;**399**(10):3307-3322. DOI: 10.1007/s00216-010-4611-x
- [8] Colwell L, Hartwick R. Non-porous silica supports for high performance liquid Chromatography. *Journal of Liquid Chromatography*. 1987;**10**(12):2721-2744. DOI: 10.1080/01483918708066822
- [9] Cheong W. Porous silica particles as chromatographic separation media: A review. *Bulletin of the Korean Chemical Society*. 2014;**35**(12):3465-3474. DOI: 10.5012/bkcs.2014.35.12.3465
- [10] Barhate C, Wahab F, Breitbach Z, Bell D, Armstrong D. High efficiency, narrow particle size distribution, sub-2 μm based macrocyclic glycopeptide chiral stationary phases in HPLC and SFC. *Analytica Chimica Acta*. 2015;**898**:128-137. DOI: 10.1016/j.aca.2015.09.048
- [11] Horvath K, Lukacs D, Sepsey A, Felinger A. Effect of particle size distribution on the separation efficiency in liquid chromatography. *Journal of Chromatography. A*. 2014;**1361**:203-208. DOI: 10.1016/j.chroma.2014.08.017
- [12] Huang M et al. Preparation of silica microspheres with a broad pore size distribution and their use as the support for a coated cellulose derivative chiral stationary phase. *Journal of Separation Science*. 2017;**41**:1232-1239. DOI: 10.1002/jssc.201701215
- [13] Qin Q, Zhang S, Zhang W, Zhang Z, Xiong Y, Guo Z, Fan J, Zheng S, Finlow D, Yin Y. The impact of silica gel pore and particle sizes on HPLC column efficiency and resolution for an immobilized, cyclodextrin-based, chiral stationary phase. *Journal of Separation Science*. 2010;**33**(17-18):2582-2589. DOI: 10.1002/jssc.200900831
- [14] Nguyen D, Guillarme D, Rudaz S, Veuthey J. Fast analysis in liquid chromatography using small particle size and high pressure. *Journal of Separation Science*. 2006;**29**:1836-1848. DOI: 10.1002/jssc.200600189
- [15] Majors R. HPLC and UHPLC Columns: Then, Now, Next, LCGC. 2018;**36**(2):128-131
- [16] Kaczmarski K, Guiochon G. Modeling of the mass-transfer kinetics in chromatographic columns packed with Shell and Pellicular particles. *Analytical Chemistry*. 2007;**79**(12):4648-4656. DOI: 10.1021/ac070209w
- [17] Wiest LA, Jensen DS, Hung CH, Oisen RE, Davis RC, Vail MA, Dadson AE, Nesterenko PN, Linford MR. Pellicular particles with spherical carbon cores and porous nanodiamond/polymer shells for reversed-phase HPLC. *Analytical Chemistry*. 2011;**83**(14):5488-5501. DOI: 10.1021/ac200436a
- [18] Staub A, Zurlino D, Rudaz S, Veuthey J, Guillarme D. Analysis of peptides and proteins using sub-2 μm and sub-3- μm shell particles. *Journal of Chromatography. A*. 2011;**1218**:8903-8914. DOI: 10.1016/j.chroma.2011.07.051
- [19] Durham D, Hurley T. Effect of sub-2-micron particle size on peak efficiency, capacity, and resolution in preparative liquid chromatography. *Journal of Liquid Chromatography and Related Technologies*. 2007;**30**:1895-1901. DOI: 10.1080/10826070701386462

- [20] Fekete S, Ganzler K, Fekete J. Facts and myths about columns packed with sub-3 μm and sub-2 μm particles. *Journal of Pharmaceutical and Biomedical Analysis*. 2010;**51**(1):55-64. DOI: 10.1016/j.jpba.2009.08.003
- [21] Olah E, Fekete S and J, Ganzler K, comparative study of new shell-type, sub-2 μm fully porous and monolith stationary phases, focusing on mass-transfer resistance. *Journal of Chromatography. A*. 2010;**1217**:3642-3653. DOI: 10.1016/j.chroma.2010.03.052
- [22] Wang Y et al. Sub-2 μm porous silica materials for enhanced separation performance in liquid chromatography. *Journal of Chromatography. A*. 2012;**1228**:99-109. DOI: 10.1016/j.chroma.2011.08.085
- [23] Wang Y, Ai F, Ng S, Tan T. Sub-2 μm porous silica materials for enhanced separation performance in liquid chromatography. *Journal of Chromatography. A*. 2012;**1228**:99-109. DOI: 10.1016/j.chroma.2011.08.085
- [24] Shaaban H, Gorecki T. Green ultra-fast high- performance liquid chromatographic method using a short narrow- bore column packed with fully porous sub-2 micron particles for the simultaneous determination of selected pharmaceuticals as surface water and wastewater pollutants. *Journal of Chromatography. A*. 2011;**1218**:252-261
- [25] Fekete S, Fekete J, Ganzler K. Shell and small particles: Evaluation of new column technology. *Journal of Pharmaceutical and Biomedical Analysis*. 2009;**49**:64-71. DOI: 10.1016/j.jpba.2008.10.009
- [26] Austin J. Ultra performance liquid chromatography(UPLC)-a review. *Journal of Analytical and Pharmaceutical Chemistry*. 2015;**2**:1056
- [27] Fountain K, Neue U, Grumbach E, Diehl D. Effects of extra-column band spreading, liquid chromatography system operating pressure, and column temperature on the performance of sub-2- μm porous particles. *Journal of Chromatography. A*. 2009;**1216**:5797-5988. DOI: 10.1016/j.chroma.2009.06.044
- [28] DeStefano J, Langlois T, Kirkland J. Characteristics of superficially-porous silica particles for fast HPLC: Some performance comparisons with Sub-2- μm particles. *Journal of Chromatographic Science*. 2008;**46**(3):254-260. DOI: 10.1093/chromsci/46.3.254
- [29] DeStefano J, Boyes B, Schuster S, Miles W, Kirkland J. Are Sub-2 μm particles best for separating small molecules? An alternative. *Journal of Chromatography. A*. 2014;**1368**:163-172. DOI: 10.1016/j.chroma.2014.09.078
- [30] Chawla G, Ranjan C. Principle, instrumentation, and applications of UPLC: A novel technique of liquid chromatography. *Open Chemistry Journal*. 2016;**3**:1-16. DOI: 10.2174/1874842201603010001
- [31] Carr P, Stoll D, Wang X. Perspectives on recent advances in the speed of high performance liquid chromatography. *Analytical Chemistry*. 2011;**83**(6):1890-1900. DOI: 10.1021/ac102570t

- [32] Moody H. The evaluation of the parameters in the van Deemter equation. *Journal of Chemical Education*. 1982;**59**(4):290. DOI: 10.1021/ed059p290
- [33] Gritti F, Guiochon G. The van Deemter equation: Assumptions, limits, and adjustment to modern high performance liquid chromatography. *Journal of Chromatography. A*. 2013;**1302**:1-13. DOI: 10.1016/j.chroma.2013.06.032
- [34] Wren S, Tchelitcheff P. Use of ultra-performance liquid chromatography in pharmaceutical development. *Journal of Chromatography. A*. 2006;**1119**(1-2):140-146. DOI: 10.1016/j.chroma.2006.02.052
- [35] Nazario C et al. Evolution in miniaturized column liquid chromatography instrumentation and applications: An overview. *Journal of Chromatography. A*. 2015;**1421**:18-37. DOI: 10.1016/j.chroma.2015.08.051
- [36] Carr P, Wang X, Stoll D. The effect of pressure, particle size and time on optimizing performance in LC. *Analytical Chemistry*. 2009;**81**(13):5342-5353. DOI: 10.1021/ac9001244
- [37] Calvet E, Bolsico C, Baeza-Baeza J, Celia M, Coque G. Description of the retention and peak profile for Chromolith columns in isocratic and gradient elution using mobile phase composition and flow rate as factors. *Journal of Chromatography*. 2014;**1**(4):194-210. DOI: 10.3390/chromatography1040194
- [38] Guiochon G, Colin H. Chapter 1 Narrow-Bore and Micro-Bore Columns in Liquid Chromatography. *Journal of Chromatography*. 1984;**28**:1-38. DOI: 10.1016/S0301-4770(08)60692-2
- [39] Ishii D, Asai K, Hibi K, Jonokuchi T, Nagaya M, A study of micro-high-performance liquid chromatography: I. Development of technique for miniaturization of high-performance liquid chromatography. *Journal of Chromatography A*. 1977;**144**(2):157-168. DOI: 10.1016/S0021-9673(00)99351-8
- [40] Berger T. Demonstration of high speed with low pressure drops using 1.8 μm particles in SFC. *Chromatographia*. 2010;**72**:597-602
- [41] Perrenoud AG, Veuthey JL, Guillaume D. Comparison of ultra-high performance supercritical fluid chromatography and ultra-high performance liquid chromatography for the analysis of pharmaceutical compounds. *Journal of Chromatography A*. 2012;**1266**:158-167. DOI: 10.1016/j.chroma.2012.10.005
- [42] Pauw R, Shoykhet K, Desmet G, Broeckhoven K. Understanding and minimizing the extra-column bandbroadening effects in supercritical fluid chromatography. *Journal of Chromatography A*. 2015;**1402**:132-137. DOI: 10.1016/j.chroma.2015.05.017
- [43] Berger T. Preliminary kinetic evaluation of an immobilized polysaccharide sub-2 μm column using a low dispersion supercritical fluid chromatograph. *Journal of Chromatography A*. 2017;**1510**:82-88. DOI: 10.1016/j.chroma.2017.06.021
- [44] Cancelliere G, Ciogli A, D'Acquarica I, Gasparrini F, Kocergin J, Misiti D, Pierini M, Ritchie H, Simone P, Vilani C. Transition from enantioselective high performance to

- ultra-high performance liquid chromatography: A case study of a brush-type chiral stationary phase based on sub-5-micron to sub-2- micron silica particles. *Journal of Chromatography A*. 2010;**1217**(7):990-999. DOI: 10.1016/j.chroma.2009.10.021
- [45] Chen Z, Agarwal A, Lambie B, Xu H, Yang Y, Zhang J, Weber SG. Speed and miniaturization improve separation and sensitivity. *Trends in Analytical Chemistry*. 2006;**25**(6):535-539. DOI: 10.1016/j.trac.2006.04.007
- [46] Ghanem A, Wang C. Enantioselective separation of racemates using CHIRALPAK IG amylose based chiral stationary phase under normal standard, non standard and reversed-phase high performance liquid chromatography. *Journal of Chromatography A*. 2018;**1532**:89-97. DOI: 10.1016/j.chroma.2017.11.049
- [47] Wang C, Ibrahim D, Ghanem A. Enantioselective separation of racemates using the sub-2 micron CHIRALPAK IG-U under normal standard, non-standard and reversed-phase high performance liquid chromatography. 2018 Manuscript accepted for publication with revision
- [48] Nguyen D, Guillaume D, Rudaz S, Veuthey JL. Chromatographic behaviour and comparison of column packed with sub-2 μm stationary phases in liquid chromatography. *Journal of Chromatography A*. 2006;**1128**:105-113. DOI: 10.1016/j.chroma.2006.06.069
- [49] Wu N, Clausen A. Fundamental and practical aspects of ultrahigh pressure liquid chromatography for fast separations. *Journal of Separation Science*. 2007;**30**:1167-1182. DOI: 10.1002/jssc.200700026
- [50] Fanali C, Fanali S. Chiral separations using miniaturized techniques: State of the art and perspectives. *Journal of Chemistry*. 2016;**56**:958-967. DOI: 10.1002/ijch.201600061
- [51] Zhang Z, Wang Z, Liao Y, Huwei L. Applications of nanomaterials in liquid chromatography: Opportunities for separation with high efficiency and selectivity. *Journal of Separation Science*. 2006;**29**:1872-1878. DOI: 10.1002/jssc.200600154
- [52] Sestak J, Moravcova D, Khale V. Instrument platforms for nano liquid chromatography. *Journal of Chromatography A*. 2015;**1421**:2-17. DOI: 10.1016/j.chroma.2015.07.090
- [53] Aturki Z et al. Current applications of miniaturized chromatographic and electrophoretic techniques in drug analysis. *Journal of Pharmaceutical and Biomedical Analysis*. 2014;**101**:194-220. DOI: 10.1016/j.jpba.2014.03.041
- [54] Grinias J, Kresge G. Miniaturizing columns and Instruments in liquid Chromatography. *LCGC*. 2017;**35**(8):515-516
- [55] Zotou A. An overview of recent advances in HPLC instrumentation. *Central European Journal of Chemistry*. 2012;**10**(3):554-569. DOI: 10.2478/s11532-011-0161-0